



Innovation, Quality and Expertise for Gas Detection.

## SureCell™ - H<sub>2</sub>S (M)

### Operating Performance

Operating Principle	3-electrode electrochemical
Gas Detected	Hydrogen Sulphide
Measurement Range	0-100 ppm
Maximum Overload <sup>2</sup>	150 ppm
Expected Operating Life	2 years in air
Output Signal	0.75 ±0.2µA per ppm
Temperature Range	Continuous: -20°C to +40°C Intermittent: -40°C to +55°C
Pressure Range	1 atm ±10%
Humidity Range (non-condensing)	Continuous: 15 - 90% RM Intermittent: 0 - 99% RM
Response Time (T <sup>5</sup> <sub>90</sub> )	<20 seconds
Baseline Offset (clean air)	<0.5ppm equivalent
Zero Shift (-40 to +55°C)	<0.4ppm equivalent
Long Term Output Drift	<2% per month
Repeatability	<±5%
Linearity	Linear ±<5%
Recommended Load Resistor	5Ω
Bias Voltage	Not required

### Intrinsic Safety Data




Maximum at 150 ppm	0.15mA
Maximum o/c Voltage	0.8V
Maximum s/c Current	<1.0A

### Physical Specification

Weight	5g (approx)
Housing Material	Noryl 110
Storage Life	6 months in sealed container
Storage Conditions	+10°C to +30°C
Orientation	Any
Warranty Period	18 months from date of despatch

### Ordering Details

Part Number	2112B2022
-------------	-----------

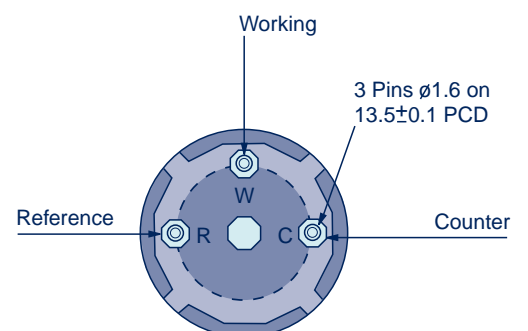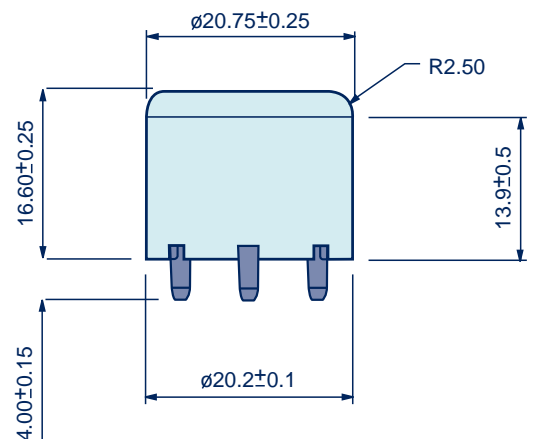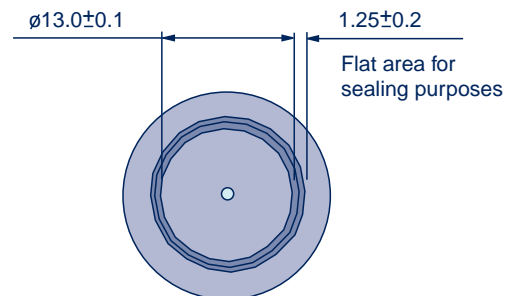





## Additional Information

Innovation, Quality and Expertise for Gas Detection.

**H2S (M) Surecell Linearity: 0 to 500ppm H2S (-1stdev)**

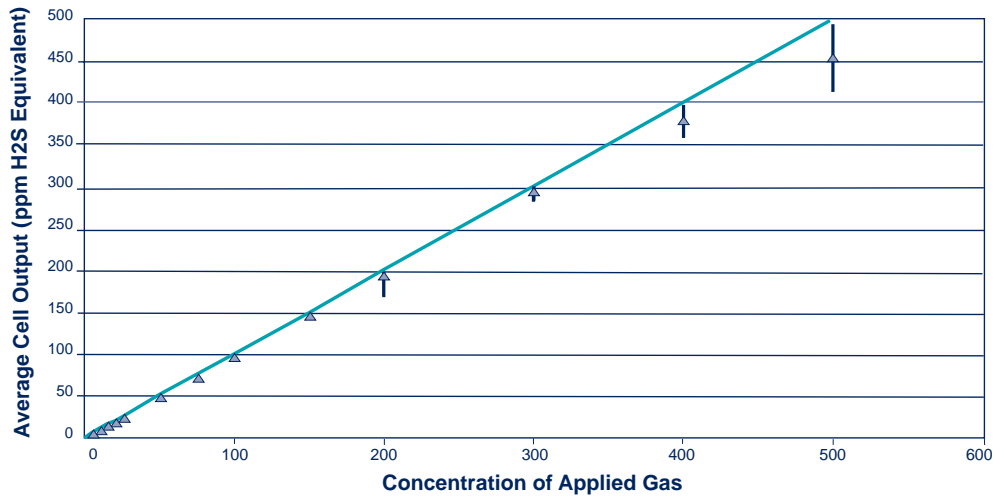

**Temperature performance of H2S (M) Surecells**

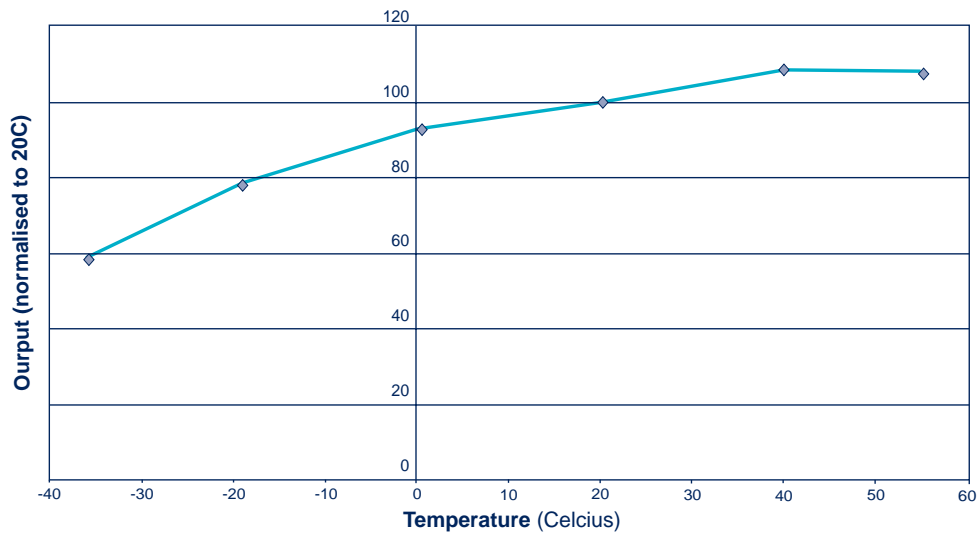

**Cross Sensitivity Table**

Gas	Concentration Used (ppm)	Reading (ppm CO)	Gas	Concentration Used (ppm)	Reading (ppm CO)
Carbon Monoxide	50	0	Chlorine	0.5	0
Hydrogen Sulphide	10	10	Hydrogen	100	0
Sulfur Dioxide	2	0	Ethylene	100	0
Nitrogen Dioxide	3	0	Carbon Dioxide	5000	0
Nitric Oxide	25	0	Ammonia	50	0

In the interest of product improvement, Sixth Sense reserves the right to alter design features and specifications without notice. Unless otherwise stated, all product specifications are quoted at standard temperature and pressure.

**\*Note:** The figures in this table are typical values and should not be used as a basis for cross calibration. Cross sensitivities may not be linear and should not be scaled. All data based on a 5 minute gassing. For some cross interferences break through will occur if gas is applied for a longer time period.